Print on Plain White Paper (Part No. 122919)

MIDMARK®

Installation Instructions

9A265002 RESTRAINT STRAP ASSEMBLY

KIT COMPONENTS

Part Number	Description	Qty.
9A265002	Restraint Strap Assembly	1
• 053-0148-00	Strap, Restraint 4" x 72" (10 cm x 183 cm)	2
• 057-0517-00	Bracket, Restraint Strap	2
• 040-0010-47	#10-24 x 3/8" Pan head phillips screw, self tapping	4
• 003-1025-00	I / O Instructions	1

REQUIRED TOOLS

Phillips Screwdriver (#2 tip)

INTRODUCTION

To confine patient to table during an examination / general procedure.

INSTALLATION (1)

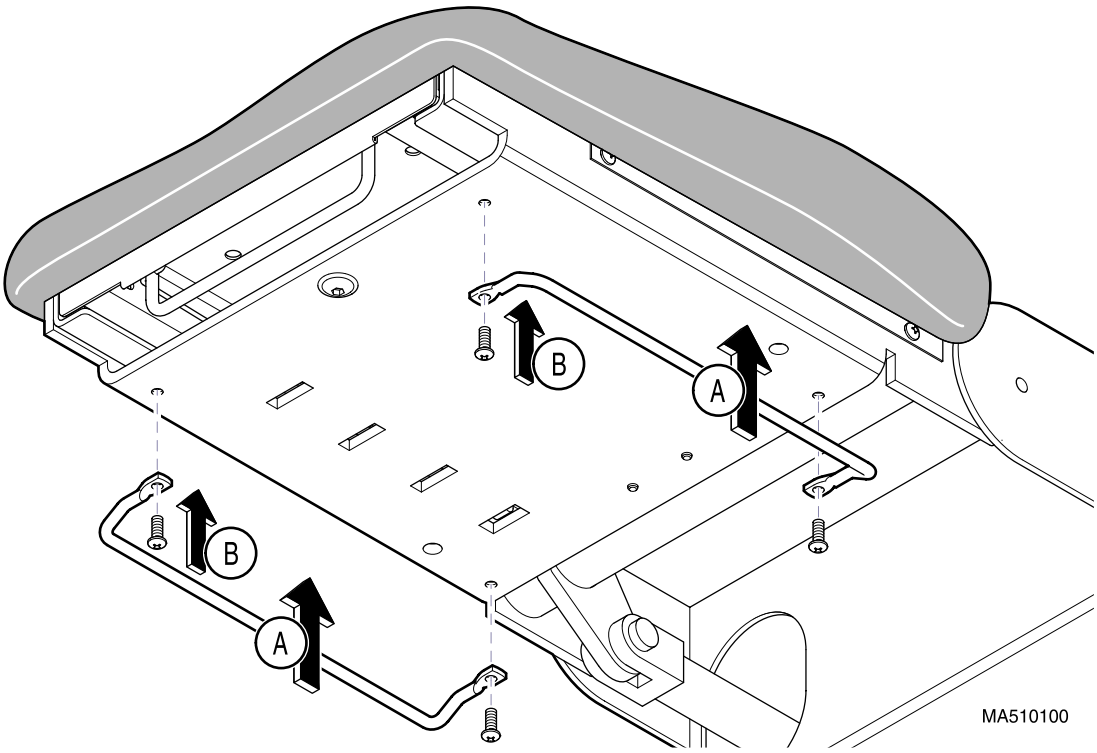

NOTE

To gain access to bottom side of Foot Assembly and mounting holes for restraint brackets., position Foot Assembly all the way upward, and Table in trendelenberg position.

A. Place Restraint Strap Brackets in position aligning holes in brackets with mounting holes in Foot Assembly.

B. Secure Brackets, using a #2 phillips screwdriver, with self tapping screws provided with assembly.

© Midmark Corporation - 1999

INSTALLATION (2)

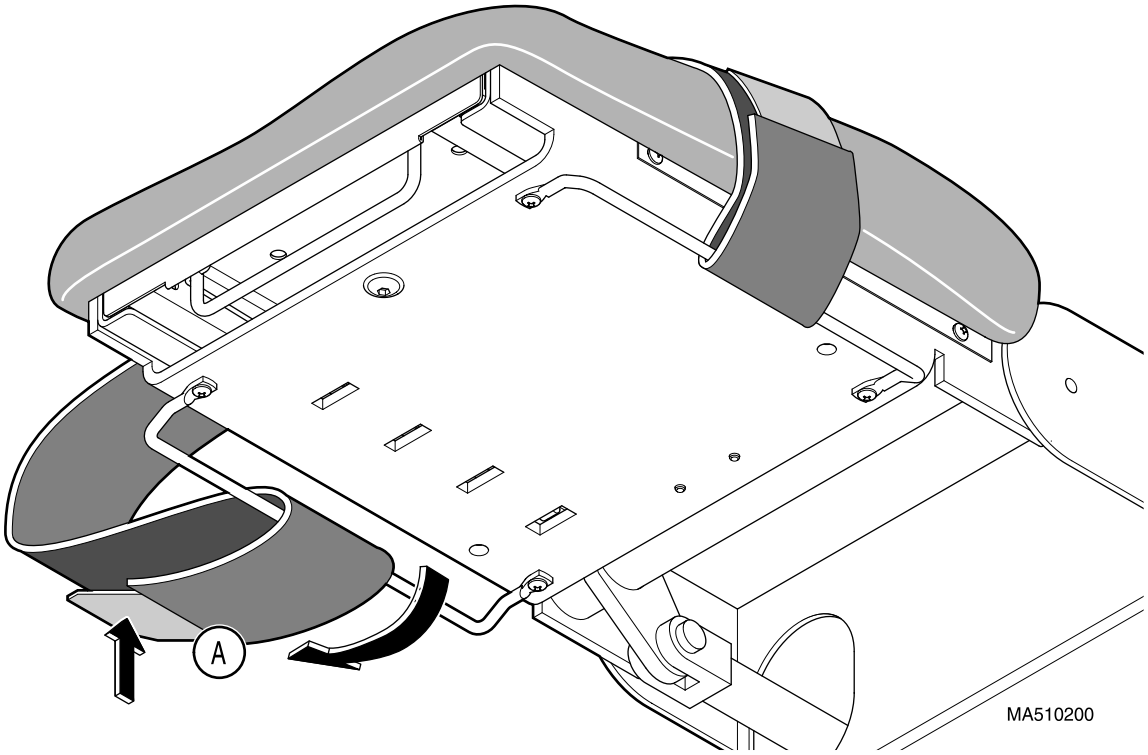

NOTE

Restraint brackets for Back Section are permanently mounted to Table Back. Restraint Straps for Back Section are mounted in same manner as Foot Section.

A. Place one end of strap through bracket, looping it so velcro contacts top of strap.

MIDMARK®

Midmark Corporation, Versailles, Ohio 45380 U.S.A.
(937) 526-3662 FAX (937) 526-5542

003-1025-00 Rev. A1 (4/99)

© Midmark Corporation - 1999